
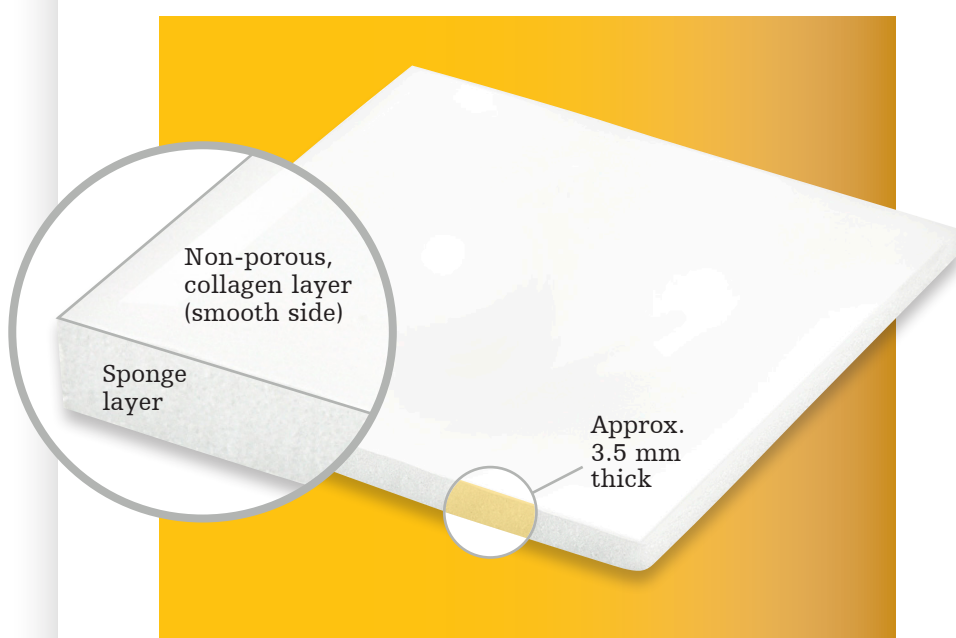


DuraMatrix-Onlay[®] Plus

Restore with confidence

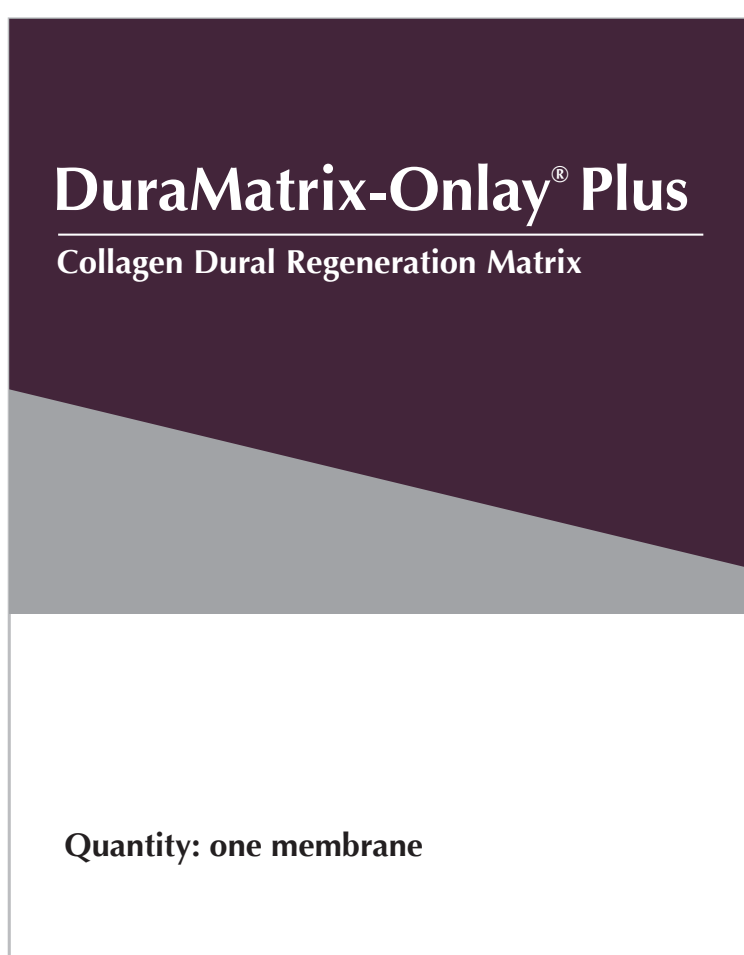

Characteristics

Application*: Onlay application. Smooth side up, sponge side down (toward the brain)

Material: Purified type I collagen derived from bovine Achilles tendon

Hydration: Prehydrate in sterile saline

Thickness: Approx 3.5mm thick

Resorption: Resorbs in approx. 8 weeks^{1,2}

Part numbers and sizes

Part number	Size	Units per
DMOP11	1 in x 1 in (2.5 cm x 2.5 cm)	1
DMOP13	1 in x 3 in (2.5 cm x 7.5 cm)	1
DMOP22	2 in x 2 in (5 cm x 5 cm)	1
DMOP33	3 in x 3 in (7.5 cm x 7.5 cm)	1
DMOP45	4 in x 5 in (10 cm x 12.5 cm)	1
DMOP57	5 in x 7 in (12.5 cm x 17.5 cm)	1

Craniomaxillofacial

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery. The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Stryker. All other trademarks are trademarks of their respective owners or holders. DuraMatrix-Onlay Plus and Dura Matrix Suturable are trademarks of Collagen Matrix, Inc. DuraMatrix-Onlay and Dura Matrix are registered trademarks of Collagen Matrix, Inc. DuraMatrix-Onlay Plus, Dura Matrix Suturable, DuraMatrix-Onlay and DuraMatrix are manufactured by Collagen Matrix, Inc., Oakland, New Jersey USA. DuraGen Plus is a registered trademark of Integra LifeSciences Corporation. Durepair is a registered trademark of TEI Biosciences, Inc.

References: 1. Rabbit duraplasty study: Data on file at Collagen Matrix, Inc. 2. The results of pre-clinical and in vitro studies may not be indicative of human clinical outcomes. *refer to respective IFUs for detailed application information.

Literature Number: CMF-PO-7_Rev. None_12686

Copyright © 2016 Stryker
UnDe/ES. Printed in the USA

Stryker Craniomaxillofacial
Kalamazoo, MI 49002 USA
t: 269 389 5346
toll free: 800 962 6558
f: 877 648 7114

stryker.com/cmf

DuraMatrix® Suturable

Restore with confidence



Characteristics

Application*: Suturable application

Material: Intact bovine dermis

Hydration: Prehydrate 1 min. in sterile saline

Thickness: Approx 1.0mm thick

Resorption: Resorbs approx 38-40 weeks^{1,2}

Part numbers and sizes

Part number	Size	Units per
DMS11	1 in x 1 in (2.5 cm x 2.5 cm)	1
DMS13	1 in x 3 in (2.5 cm x 7.5 cm)	1
DMS22	2 in x 2 in (5 cm x 5 cm)	1
DMS33	3 in x 3 in (7.5 cm x 7.5 cm)	1
DMS45	4 in x 5 in (10 cm x 12.5 cm)	1

Craniomaxillofacial

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery. The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Stryker. All other trademarks are trademarks of their respective owners or holders. DuraMatrix-Onlay Plus and Dura Matrix Suturable are trademarks of Collagen Matrix, Inc. DuraMatrix-Onlay and Dura Matrix are registered trademarks of Collagen Matrix, Inc. DuraMatrix-Onlay Plus, Dura Matrix Suturable, DuraMatrix-Onlay and DuraMatrix are manufactured by Collagen Matrix, Inc., Oakland, New Jersey USA. DuraGen Plus is a registered trademark of Integra LifeSciences Corporation. Durepair is a registered trademark of TEI Biosciences, Inc.

References: 1. Rabbit duraplasty study: Data on file at Collagen Matrix, Inc. 2. The results of pre-clinical and in vitro studies may not be indicative of human clinical outcomes. *refer to respective IFUs for detailed application information.

Literature Number: CMF-PO-7_Rev. None_12686

Copyright © 2016 Stryker

UnDe/ES. Printed in the USA

Stryker Craniomaxillofacial
Kalamazoo, MI 49002 USA
t: 269 389 5346
toll free: 800 962 6558
f: 877 648 7114

stryker.com/cmf